

Su. netrist

Tel. () 887 77

Elie
patient name

13 2017/06/02 | 08:39 AM
Age date | time

Stereo Acuity
test


Pause=0
test conditions

4.76 Meters
test distance

Quick Start
test start

2000/01/01
last calibration

Stereo Acuity

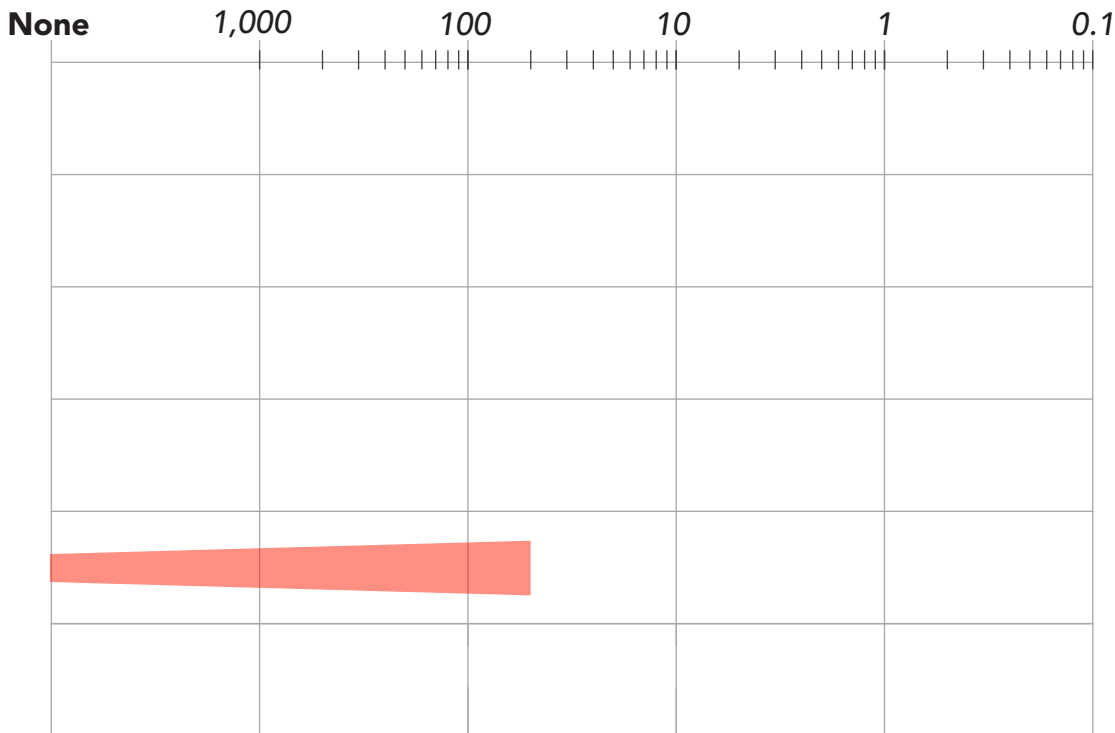

Random
Dot
Stereogram

Relative
Distance:
Three Bars

50.0
Relative
Distance:
Four Shapes

seconds of arc (log scale)



Notes: